


HER2:Cep17 RATIO

LAB	Core 1	Core 2	Core 3
116	1.3	2	0.8
140	1.52	2.86	1.1
111	1.73	3.11	1.14
113	1.85	2.69	1.07
114	1.83	3.02	1.16
115	1.6	2.6	1.2
137	1.4	2.3	1
105	1.9	3	0.96
107	1.95	3.17	1.02
108	1.4	3.9	1.1
136	1.85	2.8	1.04

May-09


ciQc Run1 ISH

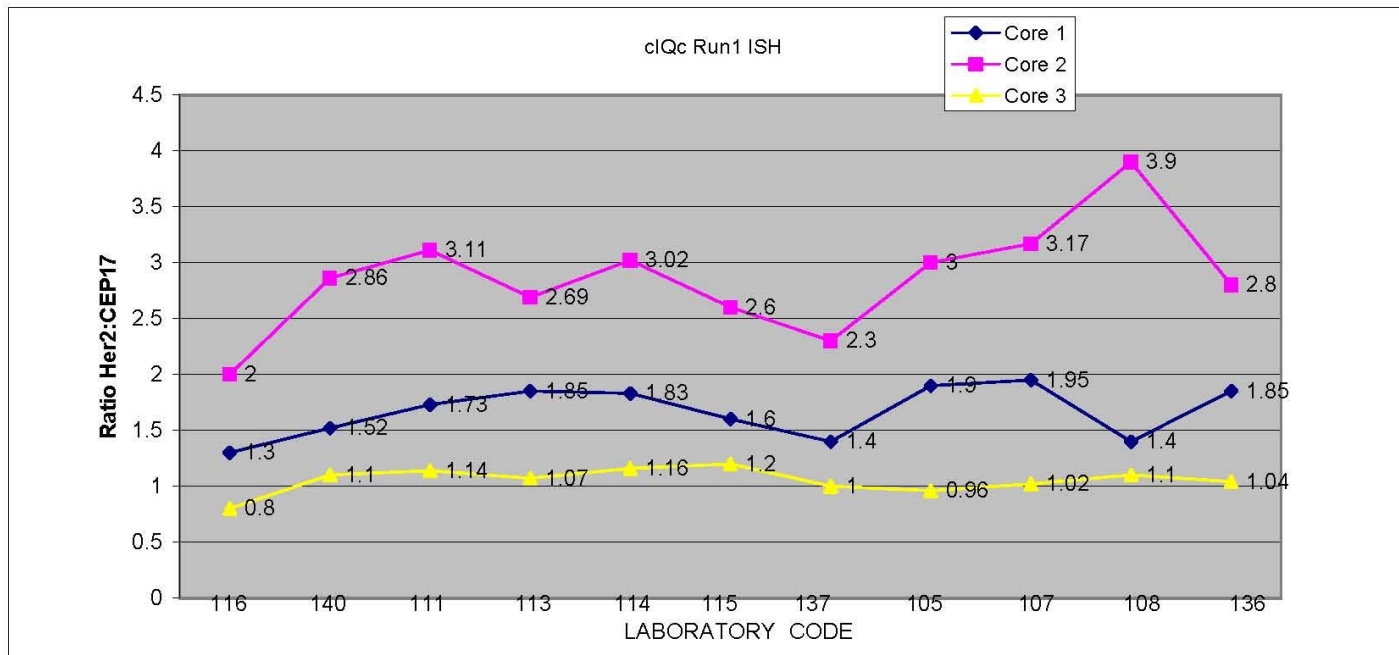

Core1

LAB	ratio	CEP17	Her2
102**			3.3
116	1.3	3.7	4.8
140	1.52	2.36	3.6
111	1.73	2.99	5.18
113	1.85	2.35	4.35
114	1.83	2.23	4.08
115	1.6	2.4	3.9
137	1.4	2.7	3.8
105	1.9	2.6	4.8
107	1.95	2.64	5.15
108	1.4	3.1	4.4
136	1.85	2.57	4.73


**site 102 uses a single probe system and cannot provide the Her2:CEP17 Ratio

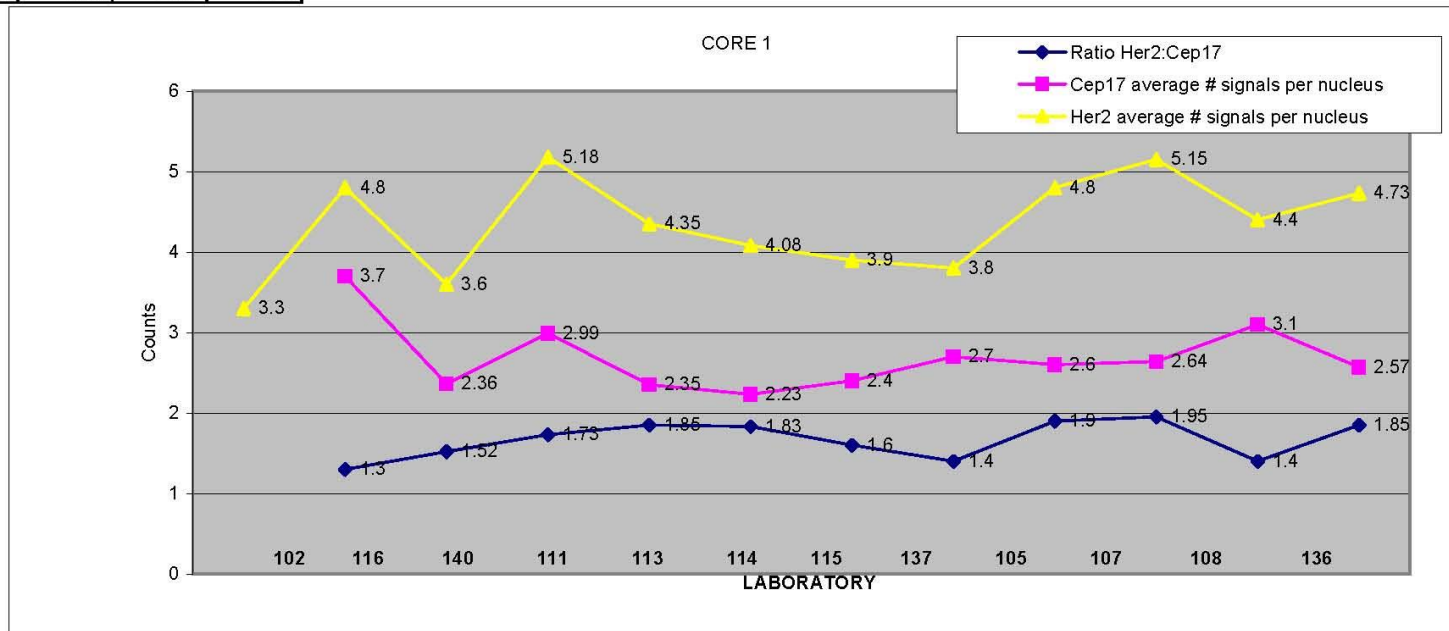

Core 2

LAB	ratio	CEP17	Her2
102**			9
116	2	4	8
140	2.86	3.6	10.5
111	3.11	3.13	9.7
113	2.69	2.4	6.45
114	3.02	2.5	7.55
115	2.6	3	7.9
137	2.3	3	6.8
105	3.3	3	10.1
107	3.17	2.63	8.35
108	3.9	2.9	11.4
136	2.8	3.2	8.97

**site 102 uses a single probe system and cannot provide the Her2:CEP17 Ratio

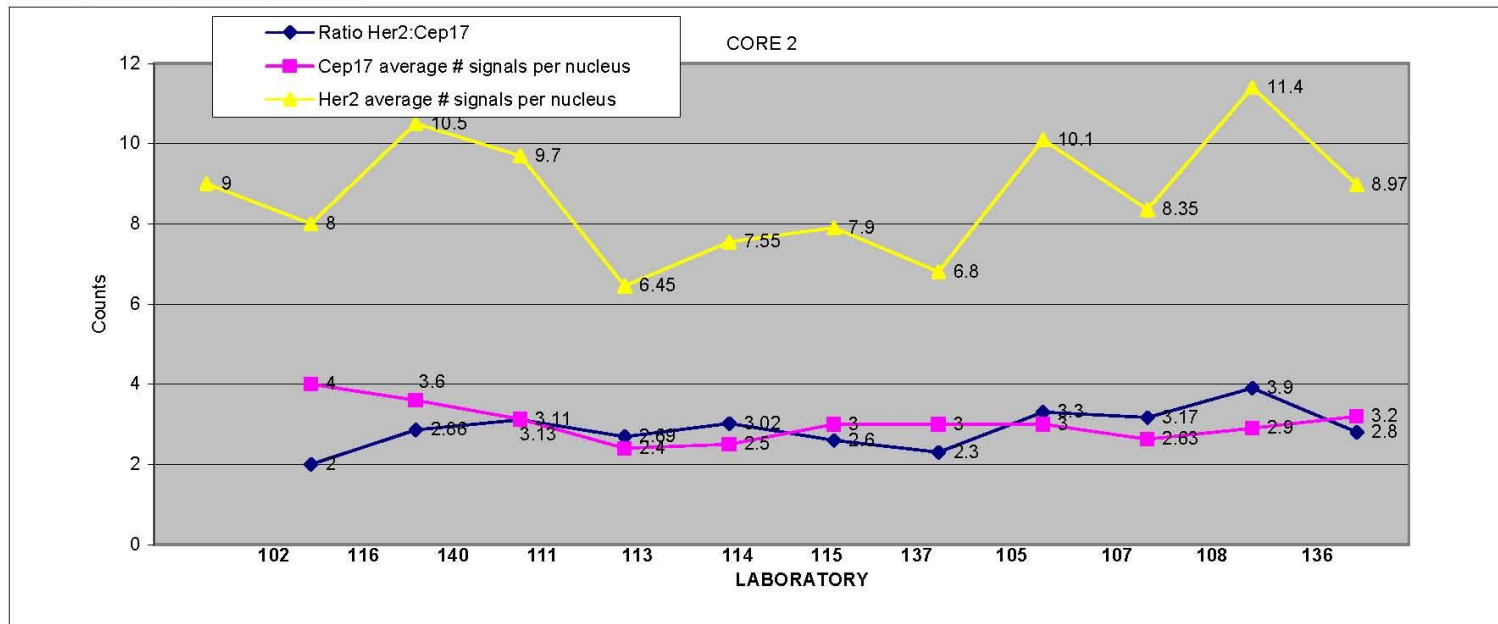

Core 3

LAB	ratio	CEP17	Her2
102**			1.8
116	0.8	1.5	1.63
140	1.1	1.95	2.17
111	1.14	2.1	2.4
113	1.07	2.1	2.25
114	1.16	1.77	2.05
115	1.2	2.8	3.3
137	1	2.1	2
105	0.96	2.56	2.44
107	1.02	1.85	1.88
108	1.1	1.4	1.5
136	1.04	2.17	2.27

**site 102 uses a single probe system and cannot provide the Her2:CEP17 Ratio

